




Publication No. 1C7070
May 1994
Supersedes 2B6835
July 1993
635883
April 1988

SITE SPECIFICATIONS

for the

Kodak RP X-Omat Processor, Model M6B

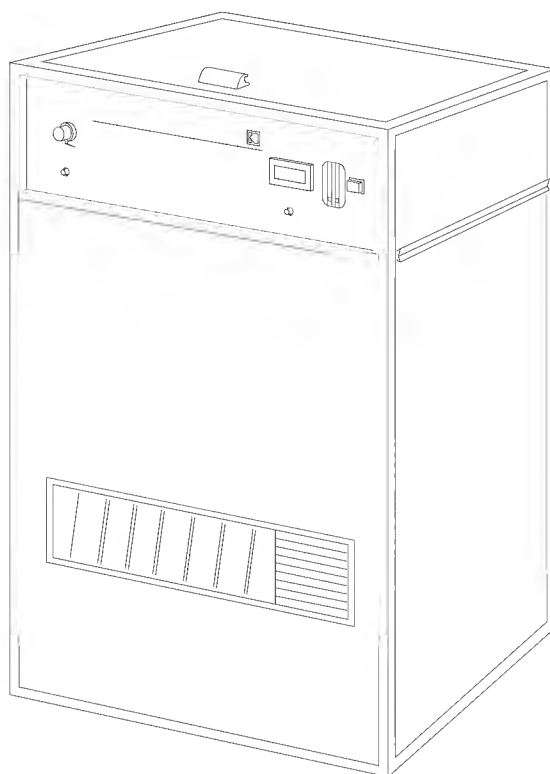

H048_0086DA

PLEASE NOTE

The information contained herein is based on the experience and knowledge relating to the subject matter gained by Eastman Kodak Company prior to publication.

No patent license is granted by this information.

Eastman Kodak Company reserves the right to change this information without notice, and makes no warranty, express or implied, with respect to this information. Kodak shall not be liable for any loss or damage, including consequential or special damages, resulting from the use of this information, even if loss or damage is caused by Kodak's negligence or other fault.

WARNING

To avoid hazardous conditions, keep floors and floor coverings around your *Kodak X-Omat* Processor and associated drains clean and dry at all times. Any accumulation of fluids from mixing tanks, drain lines, etc., should be cleaned up immediately. In the event of an accumulation of the liquid due to backup, overflow, or other malfunction of the drain associated with your *Kodak X-Omat* Processor, call a plumber or other contractor to correct any problem with your drain. Kodak accepts no responsibility or liability whatsoever for the serviceability of any drain connected to or associated with a *Kodak X-Omat* Processor. Such drains are the sole responsibility of the customer.

CAUTION

Possible damage from electrostatic discharge.

Table of Contents

| Description | Page |
|---|------|
| Introduction | 5 |
| Dimensions and Weights | 6 |
| Electrical Requirements | 7 |
| Basic Requirements | 7 |
| Standard Service Options | 7 |
| Water and Drain Requirements | 8 |
| Water Supply | 8 |
| Drain | 8 |
| Environmental Requirements | 9 |
| Room Ambient Temperature | 9 |
| Air and Heat | 9 |
| Diagrams | 11 |
| Center of Gravity | 21 |

BLANK PAGE

Introduction

This publication is part of a series of instruction books that provides technical support information on the KODAK *RP* X-OMAT Processor, Model M6B. For the ease of referencing and reordering the other publications, the following tables provide the part numbers for each of the publications.

| Publications for M6B Processors - Serial Numbers 15,000 and Above | | | | | | |
|---|-----------------|-----------------|------------|---------------------------|----------------|------------|
| | Complete Binder | Operator Manual | Site Specs | Installation Instructions | Service Manual | Parts List |
| Publication Part No. | 246630 | 1C7061 | 1C7070 | 246626 | 246628 | 246629 |

| Publications for M6B Processors - Serial Numbers 10,000 to 14,999 | | | | | | |
|---|-----------------|-----------------|------------|---------------------------|----------------|------------|
| | Complete Binder | Operator Manual | Site Specs | Installation Instructions | Service Manual | Parts List |
| Publication Part No. | 635881 | 1C7061 | 1C7070 | 635884 | 635885 | 635882 |

| Publications for M6B Processors - Serial Numbers Below 10,000 | | | | | | |
|---|-----------------|-----------------|------------|---------------------------|----------------|------------|
| | Complete Binder | Operator Manual | Site Specs | Installation Instructions | Service Manual | Parts List |
| Publication Part No. | Not Available | 1C7061 | 1C7070 | 635812 | 635828 | 635860 |

It is recommended that these publications be kept in the binder provided. If an individual document gets misplaced or destroyed, reorder a copy from your Eastman Kodak Representative.

Dimensions and Weights

Table 1 Dimensions and Weight of the Processor

| Description | Crated | Uncrated |
|--|--------------------|---|
| Length | 71.1 cm (28 in.) | 63.5 cm (25 in.) Without feed tray (Includes knobs and fittings.) 97.8 cm (38.5 in.) With feed tray (Includes dryer knob.) |
| Width | 90.2 cm (35.5 in.) | 76.2 cm (30 in.) |
| Height | 152.4 cm (60 in.) | 123.2 cm (48.5 in.) |
| Weight (Tanks Empty) | 223.2 kg (492 lb) | 201 kg (442 lb) |
| Weight (Tanks Full) | Not Applicable | 235 kg (519 lb) |
| Approximate Solution Height from the Base of the Processor | Not Applicable | 107.2 cm (42.5 in.) |

**Table 2 Maintenance and Operation
Access Requirements**

| Description | Recommendation |
|-----------------------------|-----------------------|
| Dryer End of Processor | 91.4 cm (36 in.) |
| Feed End of Processor | 91.4 cm (36 in.) |
| Drive Side of Processor | 91.4 cm (36 in.) |
| Non-Drive Side of Processor | 91.4 cm (36 in.) |
| Top of Processor | 91.4 cm (36 in.) |

Electrical Requirements

Basic Requirements

IMPORTANT

In addition, all electrical services, **including earth ground**, must comply with local and national electrical codes.

- 30 A, single-phase, 208/220, 3-wire, earth ground required.
- Main Power Disconnect (wall-mounted, not furnished)

The main power disconnect switch must consist of a minimum 2-pole thermo-magnetic circuit breaker with solid neutral and common trip, or a fused disconnect switch. This switch must be:

- located on a wall adjacent to the processor in the lighted area
- easily accessible from the processor site
- visible from the processor site.

Standard Service Options

IMPORTANT

In addition, all electrical services, **including earth ground**, must comply with local and national electrical codes.

Table 3 Service Options

| Voltage Volts | Frequency Hz | Service |
|------------------|-----------------|---------------------------|
| 100/200 | 50/60 | Single-phase, 3-wire |
| 120/208 | 60 | Three-phase*, 3-wire, Wye |
| 120/240 | 60 | Single-phase, 3-wire |
| 127/220 | 50 | Three-phase*, 3-wire, Wye |
| 220/380 | 50 | Three-phase*, 3-wire, Wye |
| 240/415 | 50 | Three-phase*, 3-wire, Wye |
| 220 | 50/60 | Single-phase, 2-wire |
| 240 | 50/60 | Single-phase, 2-wire |

*L1, L2, and Neutral used in this configuration are sometimes referred to as Single-Phase connections.

Water and Drain Requirements

Water Supply

a. Processor Supply

(1) Temperature: 4° to 29.4°C (40° to 85°F)

NOTE

If the upper limit of the room ambient or the water supply temperature to the processor is exceeded, the developer temperature may not be controlled correctly. A water chiller may be required.

(2) Pressure: 172.35 to 448.11 kPa (25 to 65 psi). Install regulator if required.

(3) Volume: Controlled within the processor to 5.7 L/min (1.5 gal/min).

(4) Filtration: A 50-micron filter is required, but it is not supplied with the processor.

b. Water service must comply with local codes.

c. Tempered water service is suggested for processor cleaning and for mixing chemicals manually.

d. A molded adapter and washer are provided to adapt the processor garden hose fitting to the 1/2 in. NPT (male).

Drain

WARNING

- Drains must be made of chemically resistant, non-corrosive material. Use PVC or the equivalent.
- The drain must have a minimum diameter of 7.6 cm (3 in.) and be free of obstruction.
- Drain service must comply with all local codes.
- Locate the drain within 1.5 m (60 in.) of the processor.
- The drain line should slope gradually downward to the floor drain.

Capacity: 15 L/min (4 gal/min).

Connection: Open drain; avoid solid connection.

Environmental Requirements

Room Ambient Temperature

- Temperature: 15° to 30°C (59° to 86°F)
- Humidity: 15% to 76%

NOTE

If the upper limit of the room ambient or the water supply temperature to the processor is exceeded, the developer temperature may not be controlled correctly. A water chiller may be required.

Air and Heat

- a. Air Exhaust (full load)
 - (1) Volume: 1.9 m³/min (65 ft³/min)
 - (2) Temperature: 66°C (150°F) maximum
 - (3) Moisture > 300 gr/min or 121 gr/kg (55 gr/lb) of air
- b. Heat load to room: 4220 kJ/hr (4000 Btu/hr)

To protect the processor and equipment directly interfaced with the processor, the dryer must be vented according to the following specifications. Failure to properly vent the dryer exhaust can cause corrosion within the processor and interfaced equipment. In addition, the probability of processor-related film artifacts is increased.


- [1] The processor exhaust duct must be connected to the building exhaust ducting system. Disposal of effluent air must comply with prevailing environmental codes.
- [2] The following table should be used to determine the proper amount of negative air within the duct at the end to be connected to the processor. To prevent venturi effect at the duct opening, all measurements should be made at a point 30.5 cm (12 in.) from the open end of the duct to be attached to the processor.

Compare the average reading with the table below.

Table 4 Static Pressures

| Duct Diameter | Negative Static Pressure, (Water Head) | |
|----------------|--|--------------------|
| | MIN | MAX |
| 76 mm (3 in.) | 0.76 mm (0.03 in.) | 1.02 mm (0.04 in.) |
| 102 mm (4 in.) | 0.25 mm (0.01 in.) | 0.51 mm (0.02 in.) |

- [3] Measurement can be made using an Air Meter, available through Service Parts Management as TL-2431. Measurement of negative air within flexible duct hoses will be simplified with the use of a modified Chemical Replenisher Check Tube P/N 592380, cut to a 30.5 cm (12 in.) straight line length, and connected to the rubber hose supplied with the Air Meter. An alternative is to use a hose support made from a straight piece of wire, such as a coat hanger, and tape the rubber hose to it.

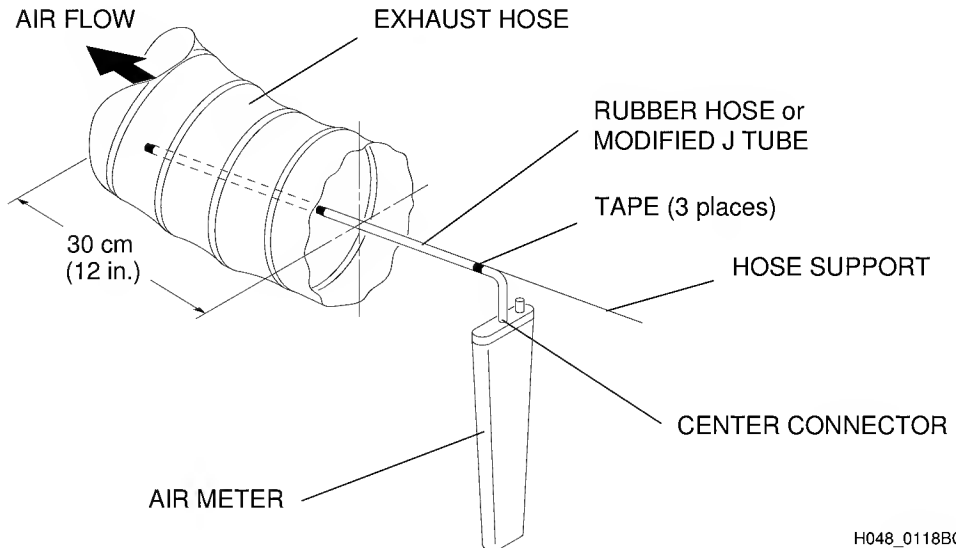

H048_0118BCA
H048_0118BA

Figure 1 Measuring Negative Static Pressure

- [4] If solid metal or rigid plastic ducting is attached to the processor in a manner which would prevent easy removal, a small hole may be created at a point approximately 30.5 cm (12 in.) from the processor vent connection. The “L” shaped metal tube provided with the Air Meter can then be inserted through the opening. When measuring negative air, the tube tip opening should be pointed in the direction of airflow away from the processor.


IMPORTANT

The processor must be turned off when making air measurements. The Air Meter should be held in the vertical position to assure the greatest accuracy. The meter tubing must not be kinked.

- [5] It is most important that negative airflow in the processor exhaust duct remains constant when the processor is in the run, standby, and shut-down modes.


When processors are installed in darkroom wall openings, it is most important that darkroom air pressure exceeds the air pressure of the area surrounding the darkroom. This is intended to prevent air cascading through the processor into the darkroom area. Proper balancing of dark/lighted room air in addition to correct dryer venting will not only maximize containment of chemical fumes and vapors within the processor and its dryer exhausting system, but the incidence of film artifacts occurring in the out-of-solution transport roller sections will be greatly reduced.

Diagrams

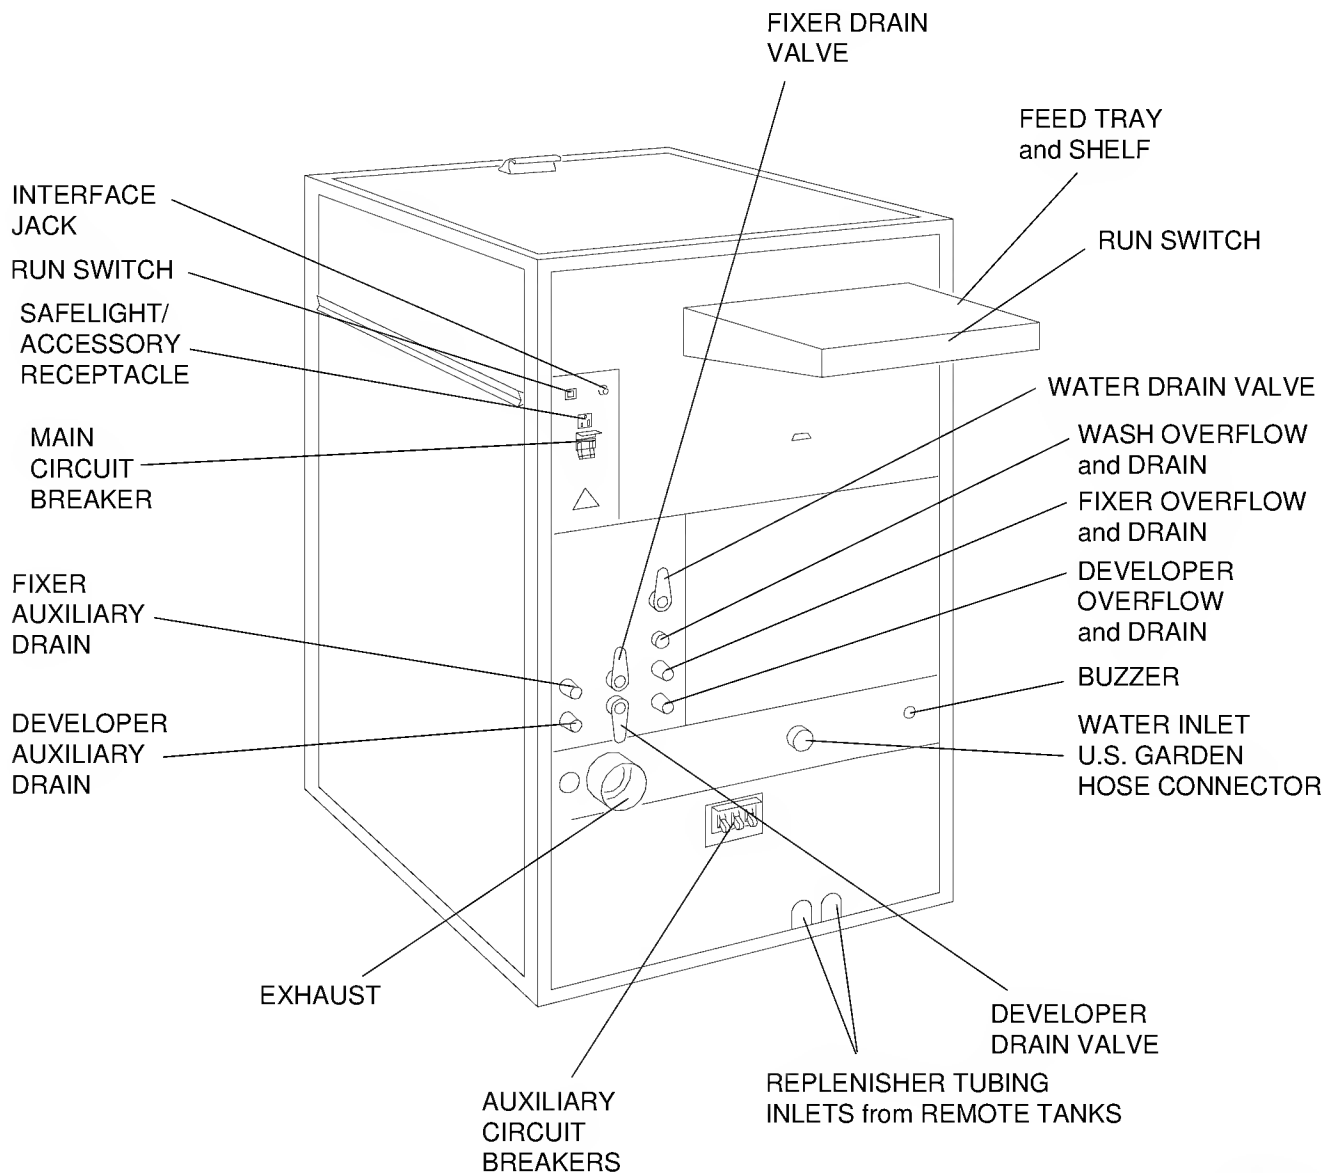


H048_0085DCA
H048_0085DA

Figure 2 Feed-End View of the Processor

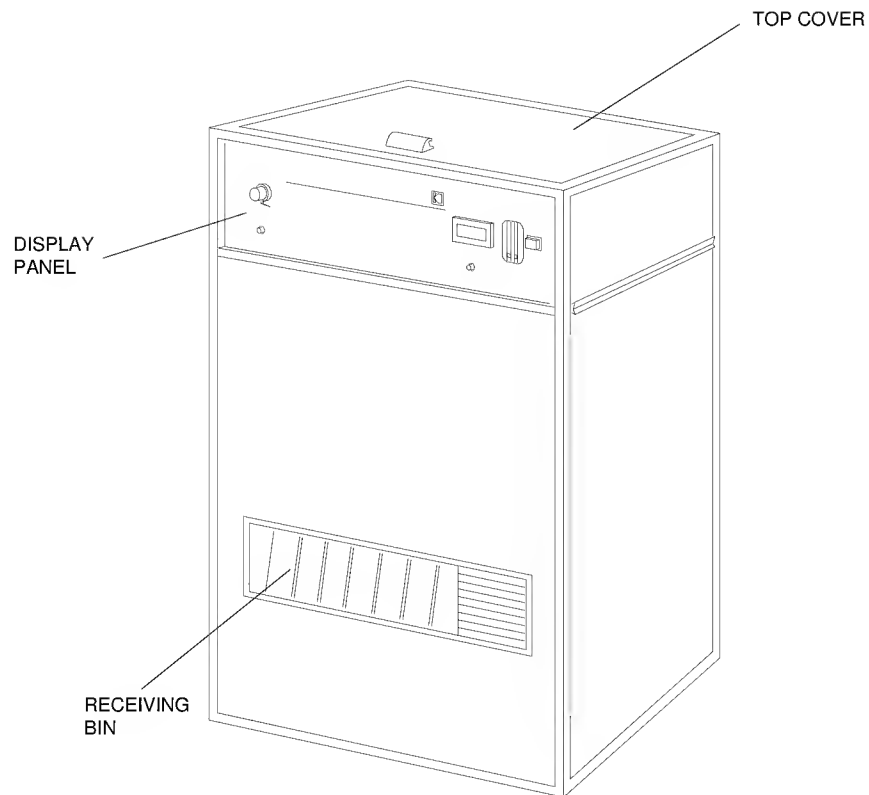


H048_0086DCA
H048_0086DA

Figure 3 Receiving-End View of the Processor

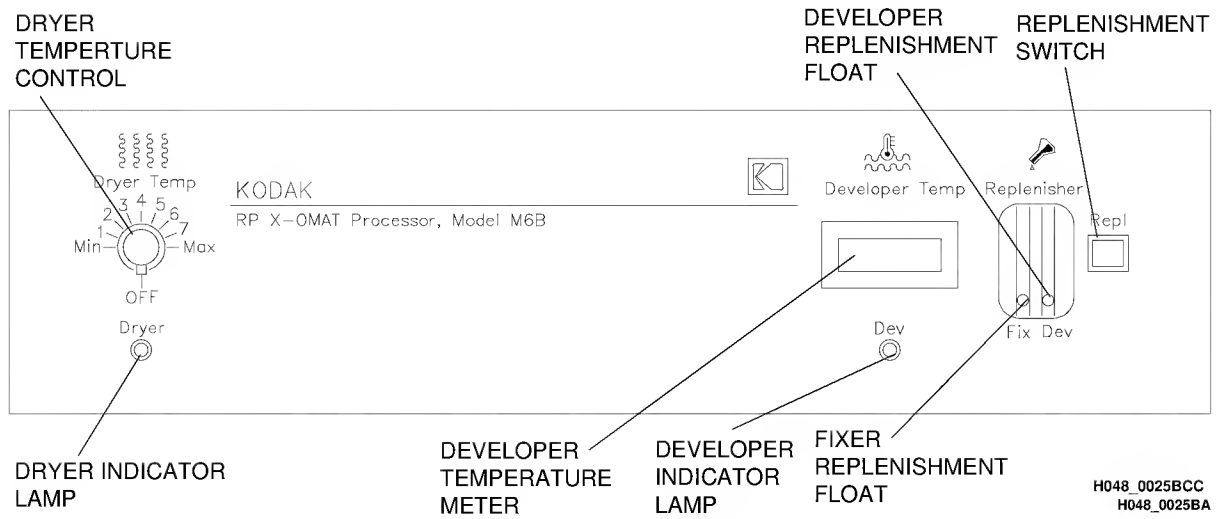


H048_0025BCC
H048_0025BA

Figure 4 Display Panel on Receiving-End of the Processor

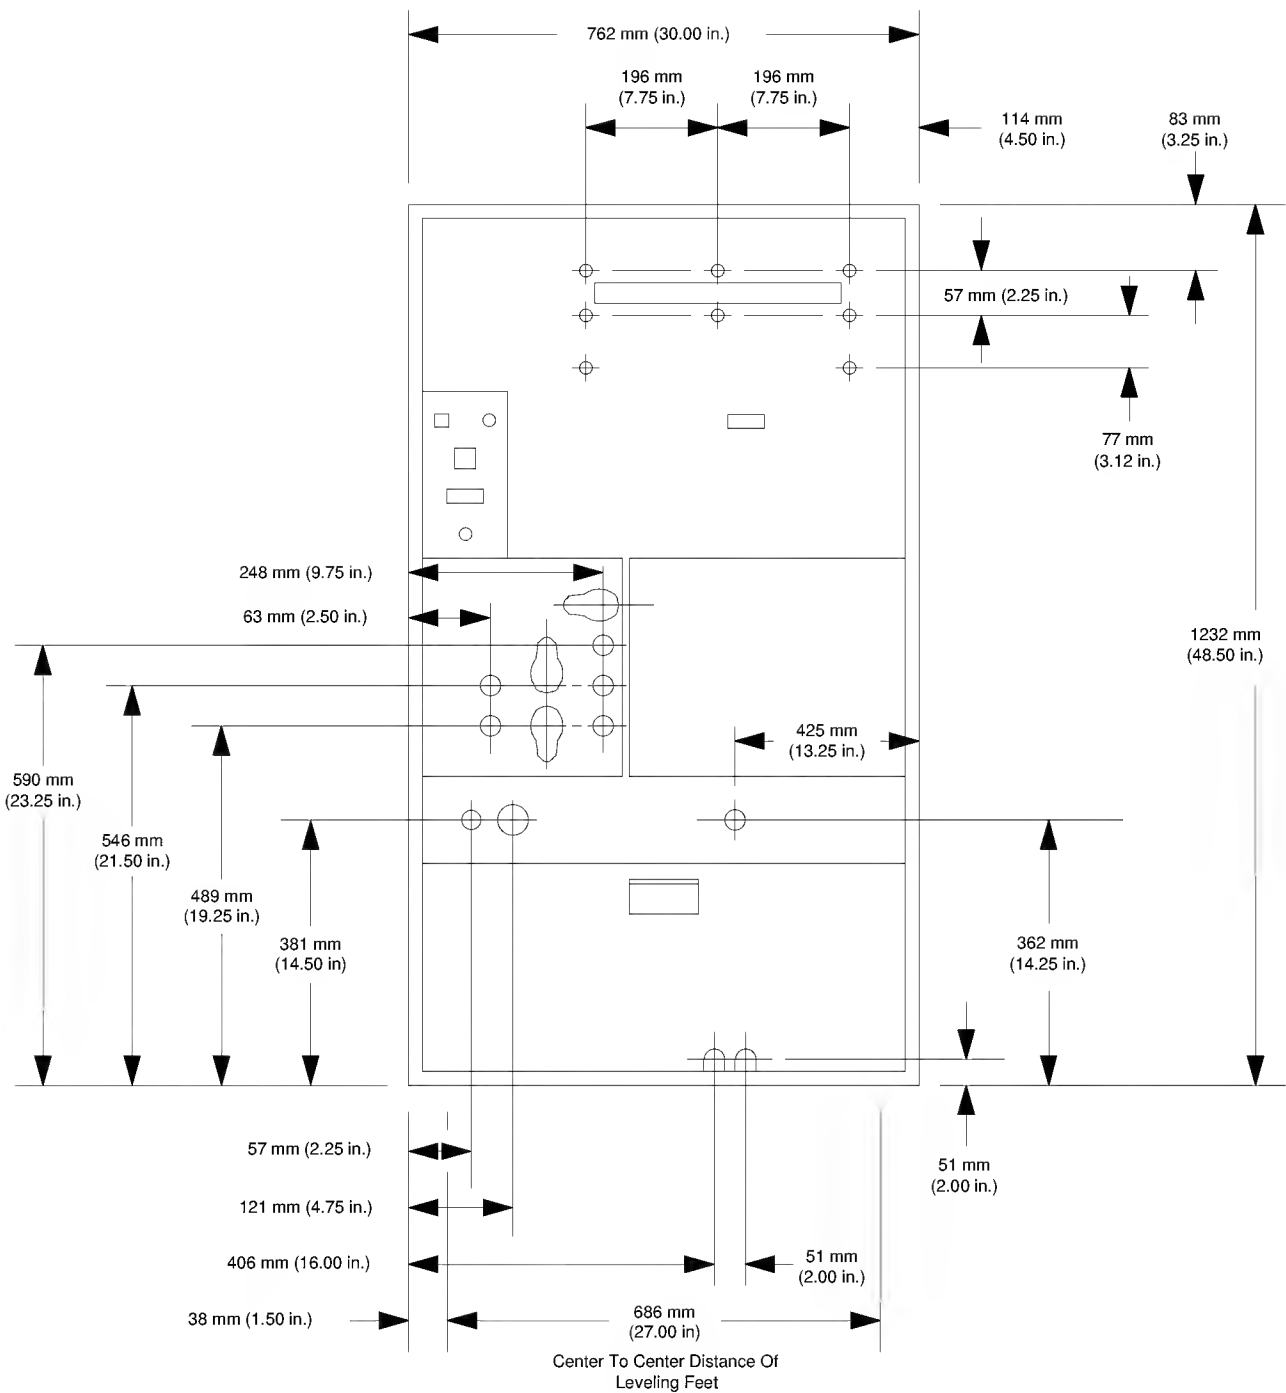

H048_0121EC

Figure 5 Feed-End Dimensions of the Processor

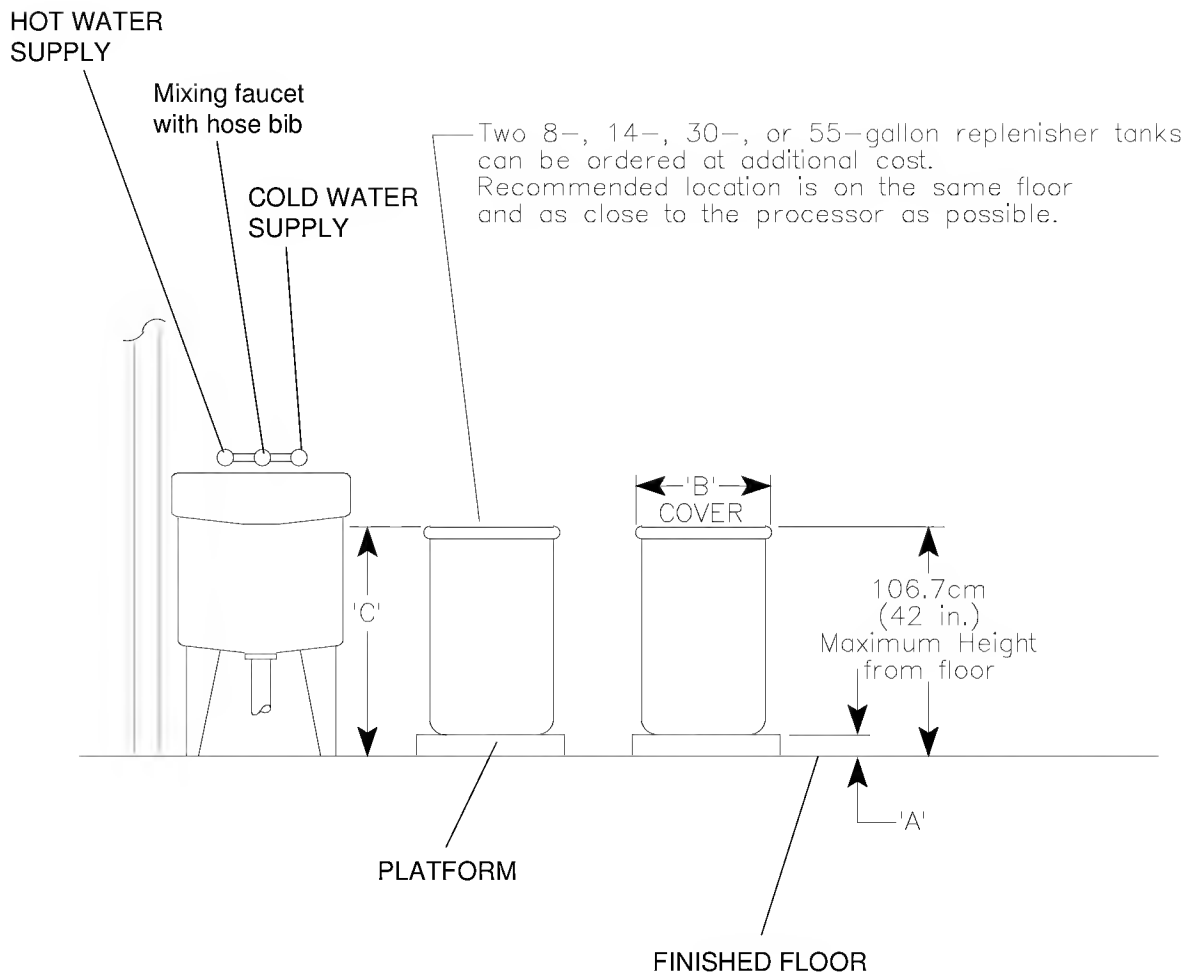


H048_0120DCA
H048_0120DA

Figure 6 Replenisher Tanks

Table 5 Dimensions for Replenisher Tanks

| DESCRIPTION | DIMENSION | 14 GAL | 30 GAL | 55 GAL |
|----------------------------------|-------------------------|-------------------------------|-------------------------------|-------------------------------|
| Max Platform Height | "A" Fig. 14 | 48.3 cm (19 in.) | 35.6 cm (14 in.) | 15.2 cm (6 in.) |
| Tank Diameter | "B" Fig. 14 | 43.2 cm (17 in.) | 55.9 cm (22 in.) | 61.0 cm (24 in.) |
| Tank Height | "C" Fig. 14 | 58.4 cm (23 in.) | 70.5 cm (27.75 in.) | 90.8 cm (35.75 in.) |
| External Replenishment Tank Area | "D" x "E" (MIN) Fig. 15 | 61.0 X 127.0 cm (24 X 50 in.) | 61.0 x 152.4 cm (24 x 60 in.) | 66.0 x 172.7 cm (26 x 68 in.) |

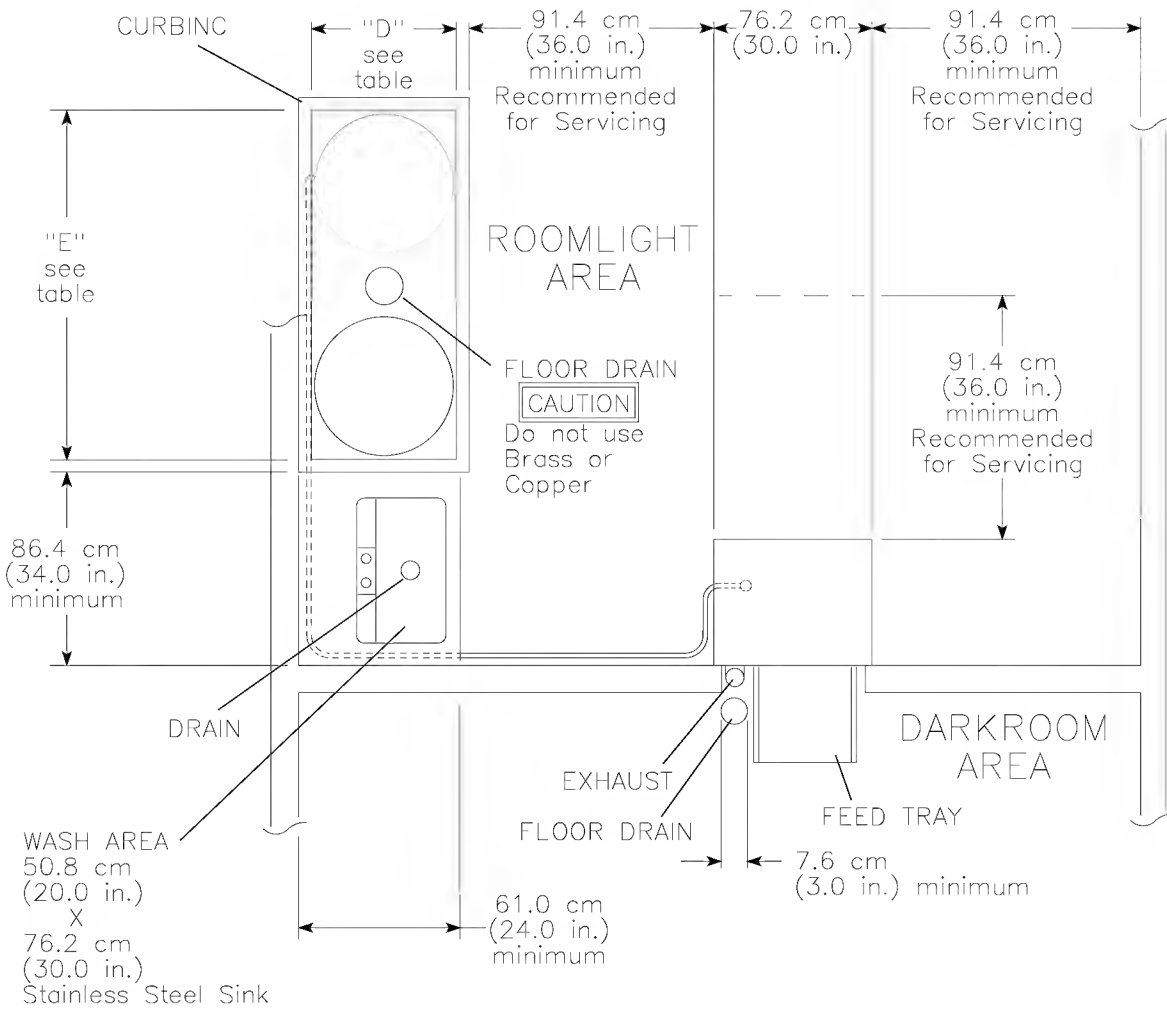


H108_0006DA

Figure 7 Suggested Room Layout and Drain Locations


Table 6 Maintenance and Operation Access Requirements

| Description | Recommendation |
|-----------------------------|------------------|
| Receiving-End of Processor | 91.4 cm (36 in.) |
| Feed-End of Processor | 91.4 cm (36 in.) |
| Drive-Side of Processor | 91.4 cm (36 in.) |
| Non-Drive Side of Processor | 91.4 cm (36 in.) |
| Top of Processor | 91.4 cm (36 in.) |

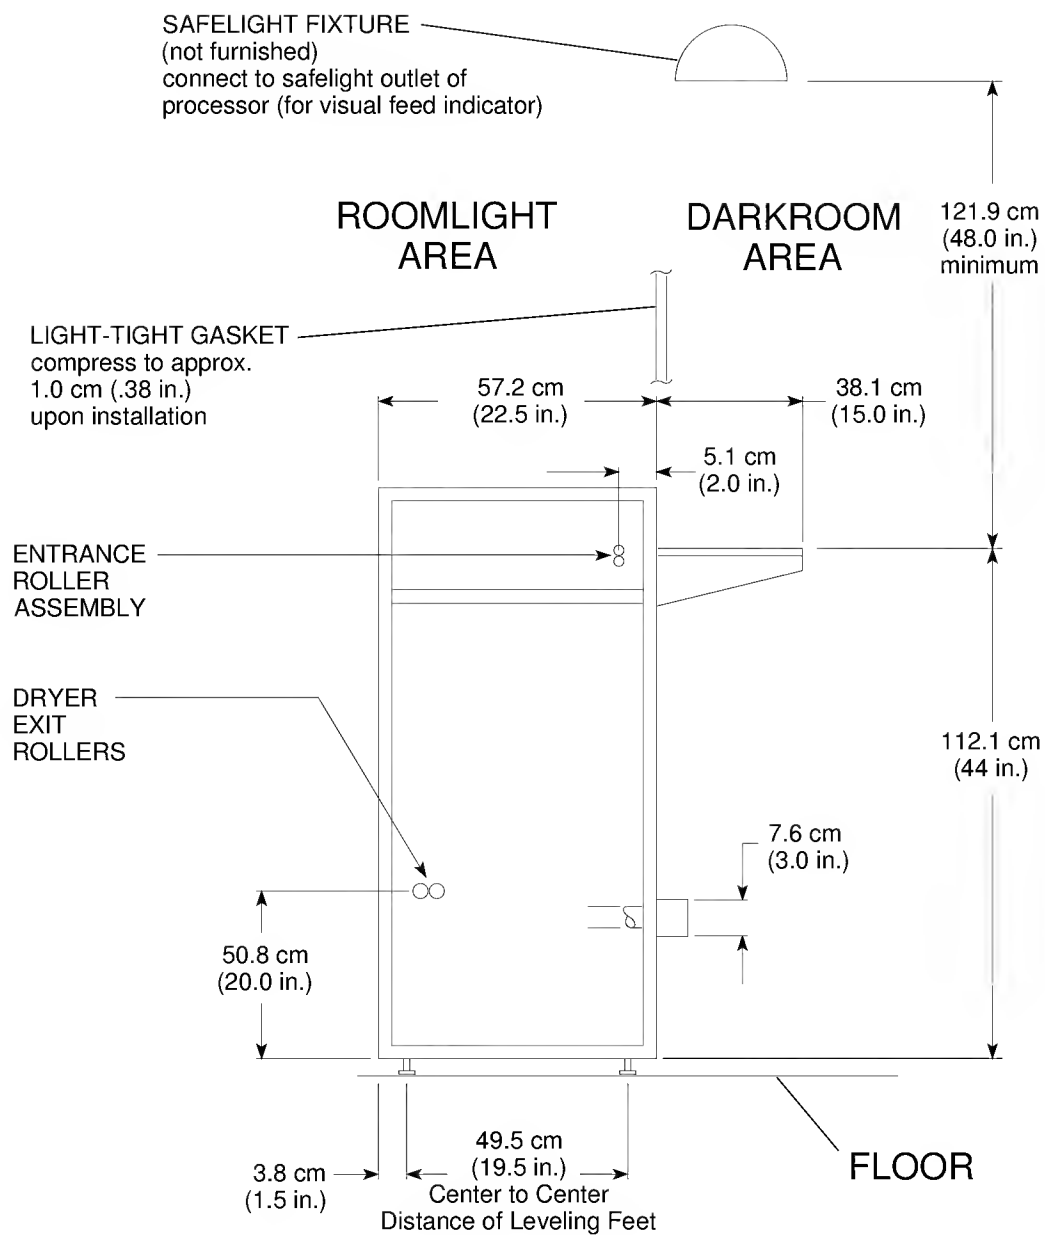

H048_0090DA

Figure 8 Side Dimensions

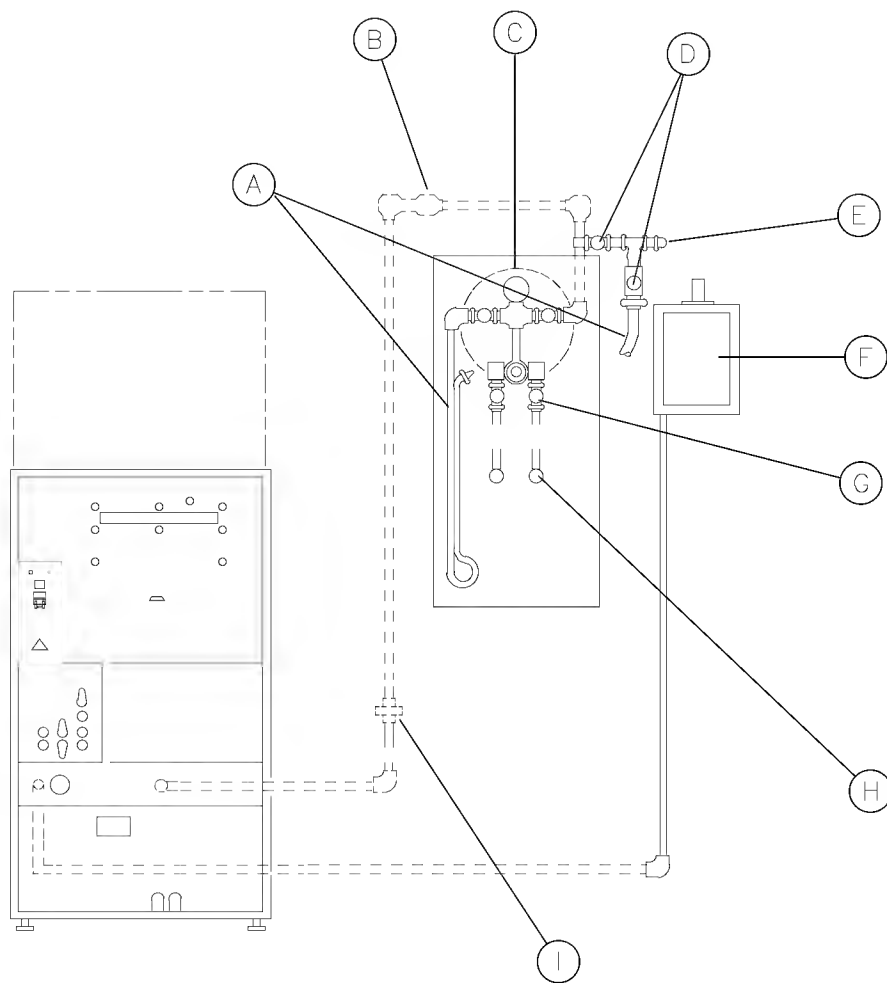

H108_0009DAA
H048_0089DA

Figure 9 Electrical and Water Connections

NOTE


- Pass service through the wall to the feed-end of the processor in the darkroom. Service controls may be located on either side of the processor for easy accessibility.
- See the Table on page 18.

Table 7 Electrical and Water Connections, Continued

| | |
|---|---|
| A | Service Hose - suggested length to reach the Processor and Replenisher Tanks. |
| B | ½ in. NPT Check Valve |
| C | <p>Kodak Thermostatic Mixing Valve ½ in. NPT available from Eastman Kodak Company, Part No. 467621. Not supplied with the Processor.</p> <p style="text-align: center;">IMPORTANT</p> <p>A mixing valve is not required for the processor if incoming water temperature is between 4° and 29.4°C (40° and 85°F).</p> |
| D | Shutoff Valves ½ in. NPT. Two additional required. Available from Eastman Kodak Company, Part No. 459981. Not supplied with the Processor. |
| E | Cold Water Supply ½ in. NPT |
| F | 30 AMP - 2 POLE, Thermo-magnetic Circuit Breaker. Locate safe distance from water service. Not supplied with the Processor. |
| G | Shutoff Valves ½ in. NPT. Two additional required. Available from Eastman Kodak Company, Part No. 459981. |
| H | Hot and Cold Water Supply ½ in. NPT. |
| I | ½ in. NPT Union. Locate as close to the Processor as possible. |

NOTE

- The processor is UL listed, CSA certified. Specifications are subject to change without notice.
- Follow local electrical and plumbing codes.

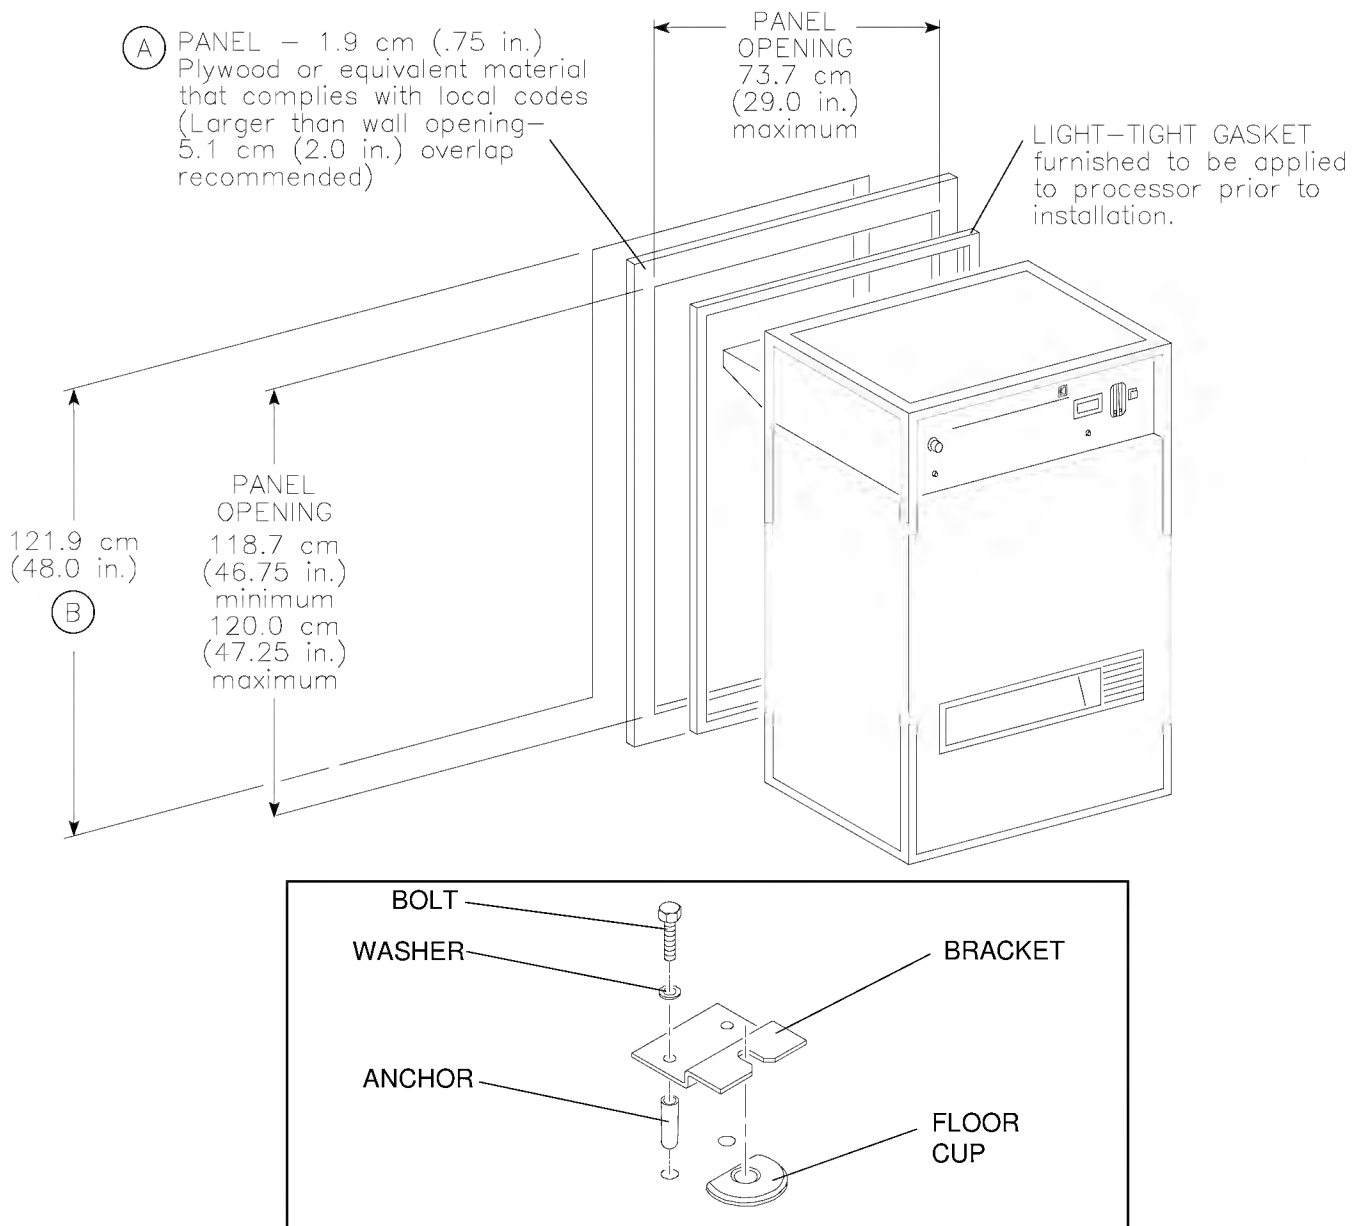

H048_0005DCA
H048_0005DA

Figure 10 New Wall Installation

- A** If the wall around the opening is straight and exactly perpendicular to the floor, this panel may not be necessary. The wall opening dimensions should match the inside dimensions of the panel opening.
- B** Make sure that the vertical dimension of $48 \pm 1/16$ in. for the wall opening is measured from the finished floor.


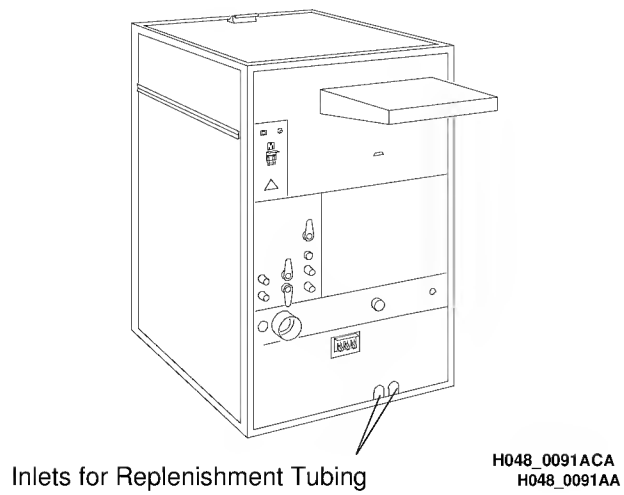



Figure 11 Inlets for Replenisher Tubing

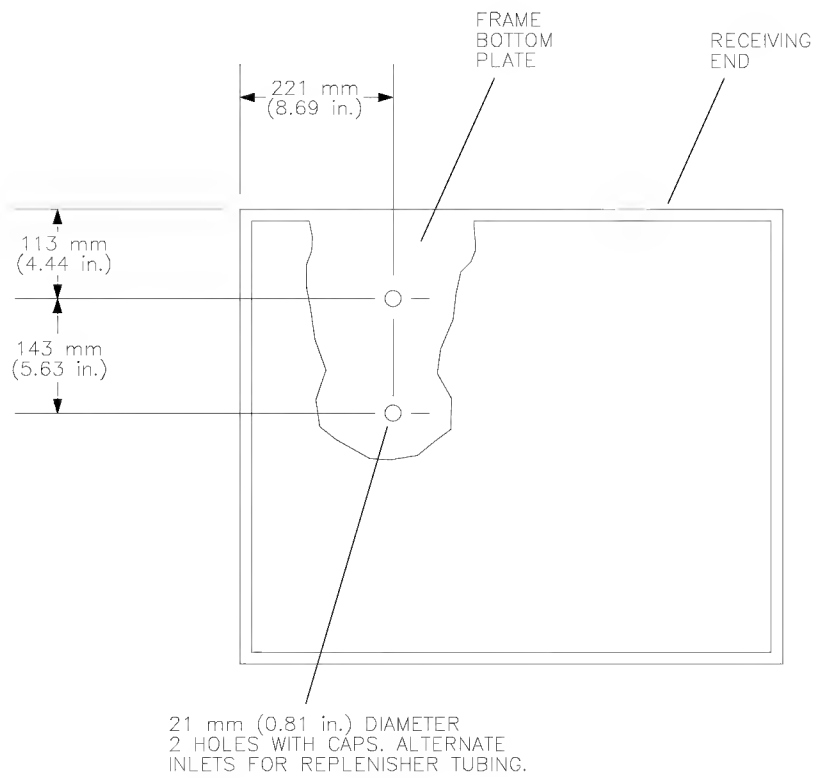

H048_0006DA

Figure 12 Alternate Inlets for Replenisher Tubing

Center of Gravity

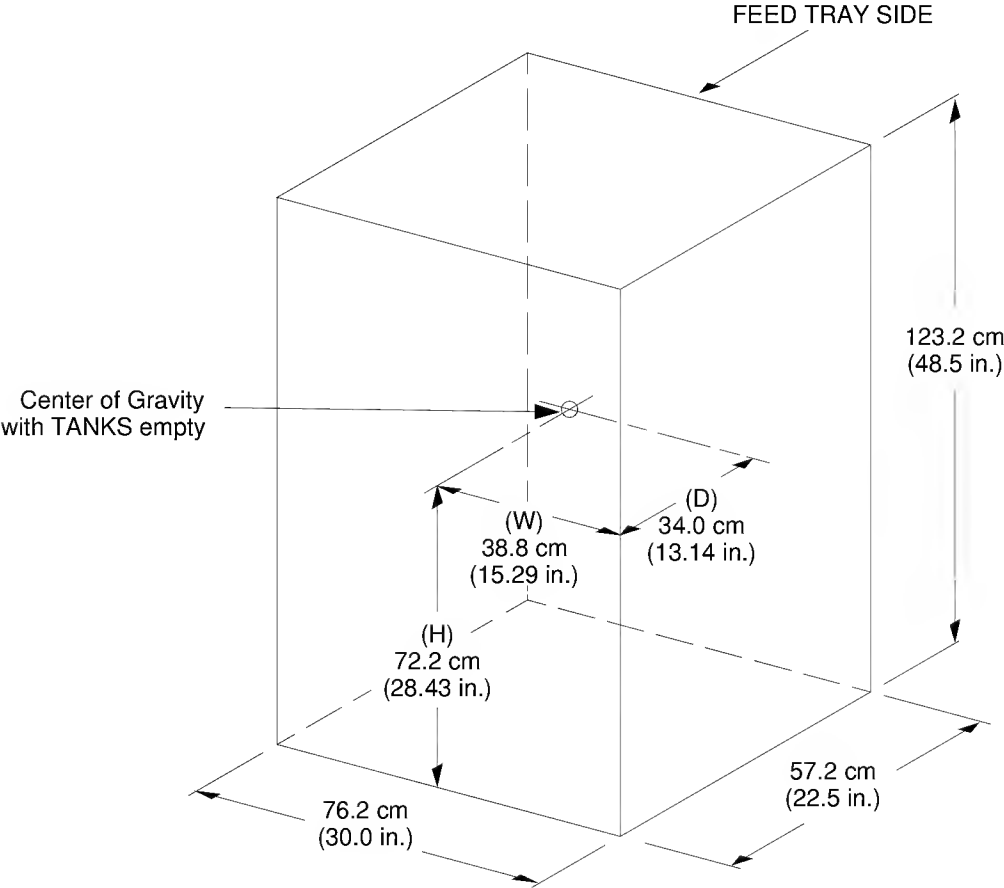

H048_0117DA

Figure 13 Center of Gravity

NOTE

Center of gravity is shown for the processor with the DEVELOPER, FIXER, and WASH TANKS empty.

3040SS_B.TXT

Kodak and X-Omat are trademarks.

Printed in USA

EASTMAN KODAK COMPANY • ROCHESTER, N.Y. 14650

Health Sciences Division

